

 mitoredlight

USER MANUAL

1070nm Intranasal Unit

www.mitoredlight.com

© 2024 MRL IP Holdings LLC. All rights reserved.

CONTENTS

Introduction	03
What's included	05
Instructions	05
Specifications and disposal	08
Cautions and disclaimer	09
Warranty and maintenance	10
About us	11

INTRODUCTION

The MitoMIND 1070nm intranasal unit, allows you to bypass the skull in delivering 1070nm near infrared light to the brain. Combined with the MitoMIND 810nm Helmet, you get the two best brain health wavelengths, in two distinct delivery routes.

To ensure the longevity of your device, please read the below cautions and disclaimers. Further disclaimers and warranty information can be found at the end of this user manual:

Please avoid subjecting the therapeutic device to strong shocks and extremely high temperatures.

This machine uses a specific charger, so it is strictly prohibited to use a power supply with higher voltage for charging.

After charging is complete, disconnect the charging cable to prevent potential accidents caused by prolonged charging.

Please keep liquids out of the main unit to prevent damage to internal components.

Nasal probes may develop skin allergies or irritation if exposed to soap, sweat, allergens, or contaminants for extended periods.

Please do not attempt to disassemble, repair, or modify this machine yourself.

Avoid contact with chemicals such as gasoline, cleaning solvents, propanol, alcohol, or insect repellent.

INTRODUCTION

The nose is a crucial part of the respiratory system connected to the lungs. Inflammation caused by pathogenic bacteria and viruses in the nose can spread to other areas, leading to complications in the brain, eyes, ears, throat, and lungs.

This nasal cavity therapeutic instrument utilizes a 1070 nm soft laser to repair damaged nasal mucosa tissue, enhance detoxification metabolism and the natural immune response of nasal tissue, accelerate capillary blood circulation in the mucosa, and boost the bactericidal activity of phagocytes. It helps reduce nasal tissue swelling, improve nasal airflow, decrease histamine release from mast cells, and alleviate nasal allergic reactions.



Warning:

Do not shine the nasal probe directly into your eyes.

WHAT'S INCLUDED



Main panel



Sleeve charge line



Nasal probe silicone



Packing case




Nasal irradiation probe



Manual



INSTRUCTIONS

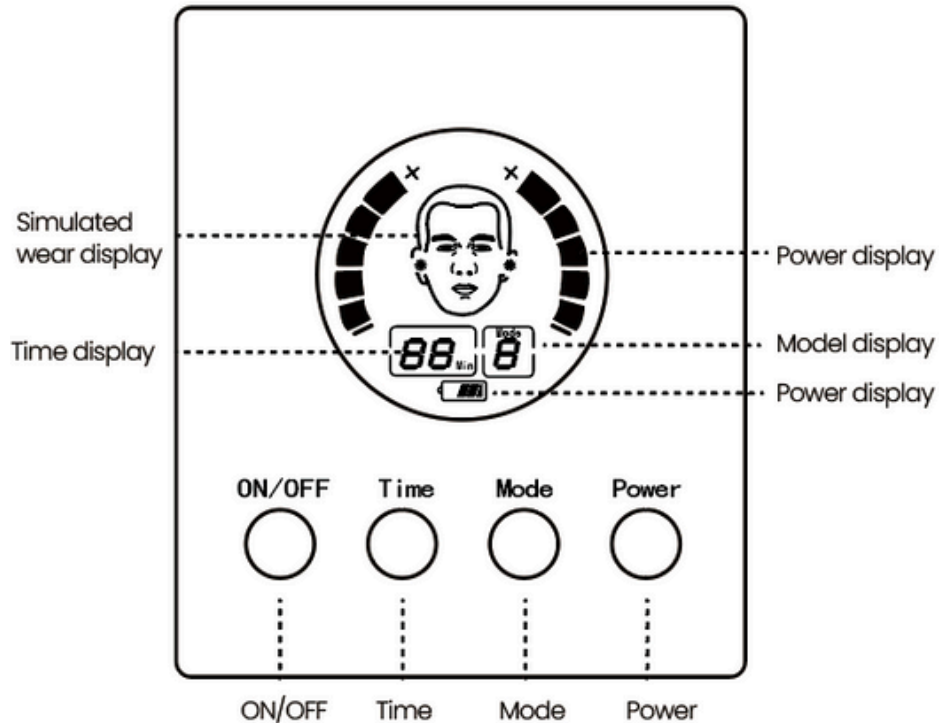

Before using the nasal irradiation probe, remove the silicone sleeve of the nasal probe from the packaging box and insert it into the irradiation probe. See Figure ①.

Once the assembly is complete, connect one end of the nasal irradiation probe to the control main unit, and insert the other end into the nasal cavity. See Figure ②.

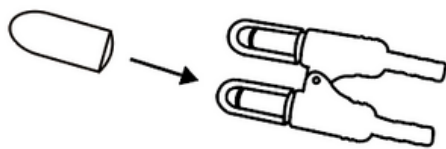


Figure ①



Figure ②

INSTRUCTIONS CONTINUED

Next, power on your device by pressing on the ON/OFF button for two seconds, then select the amount of time you would like to use the unit for.

Next, you will need to select a mode. Press the MODE button until you see your desired mode. M1 is recommended for general use.

M1 - two lights are on

M2 - only left light on

M3 - only right light on

Once the model is selected, press POWER to start your session. To end your session early, press the POWER button.

Please note, as 1070nm is past the visible spectrum it may be hard to see the light. Please do not look at the nasal probe to verify the light is on. If you would like to confirm the light is coming out, use your cell phone and take a picture of the nasal probe in a dark environment.

General usage:

We recommend starting off a lower time limit of up to 15 minutes once a day, and over the space of two weeks build your time up to 15 to 30 minutes once a day. We do recommend taking one day off per week. If you have any unwanted effects, discontinue use and contact customer service.

Charging:

When the power battery displays low battery, it is time to recharge your unit. Use the provided USB cord and connect to a USB charger (not provided) to charge your unit to full charge and then remove from the charger to preserve the life of your unit.

SPECIFICATIONS AND DISPOSAL

- Laser medium | QSI
- Laser wavelength | 1070nm
- Terminal laser output | 2 nasal cavity laser beams
- Laser output power | 2-5 mw
- Laser operating voltage | 3.7V
- Input voltage of power | 5V switching adapter
- Timing range | 15-60 minutes that can be adjusted
- Environment temperature | 20°C - 40°C
- Relative humidity | ≤85%
- Atmospheric pressure | 86 kpa – 106 kpa
- Power source use | Lithium ion battery with the capacity 1600 m Ah
- Lithium battery voltage | DC 3.7V - 4.2V

Disposal

Before disposing of the appliance, remove the battery from the device by following these steps: tear off the bottom pad, unscrew the bottom cover plate, and carefully extract the battery, ensuring to avoid short-circuiting the positive and negative poles.

Ensure the appliance is powered off before removing the battery, and dispose of it safely.

It is forbidden to throw the device into a fire to prevent it from exploding.

CAUTIONS & DISCLAIMER

Disclaimer

The statements in this manual have not been evaluated by the Food and Drug Administration (FDA). The information provided is not intended to diagnose, treat, cure, or prevent any disease and should not be construed as medical advice. Our products are low-risk, general wellness / fitness products that do not require FDA clearance, in accordance with the "General Wellness: Policy on Low Risk Devices" draft released January 20, 2015.

Mito Red Light makes no claims or representations or otherwise warranties regarding the ability of this product to cure any physical or mental conditions. A qualified health professional should always be consulted prior to using this product in regards to any condition that may requires medical attention.

WARRANTY AND MAINTENANCE

Under normal use this product is guaranteed for 1 year after its original purchase date against manufacturing defects in materials or workmanship. This warranty extends only to the original purchaser. If the product should become faulty within the warranty period, contact Mito Red Light. Mito Red Light reserves the right to repair a defective product. Mito Red Light reserves the right to replace a defective product with the most compatible product currently available.

This warranty does not cover damage caused by the following:

- Accident, misuse, abuse or alteration
- Servicing by unauthorized persons
- Connection to incorrect power sources
- Use with unauthorized accessories

Mito Red Light shall not be responsible for any incidental, special or consequential damages resulting from the use of this product.

MAINTENANCE

- This device has no serviceable parts. The battery is not accessible and not serviceable. Users should not attempt to service the battery as this will damage the device and void the warranty.
- Charge the device only with the supplied USB-C power charging cord and a universal USB-C power adapter (not included).
- The battery capacity grid will begin to flash when battery levels are low. This indicates the device should be recharged.
- The lifetime of the Lithium Ion Battery can be maximized by allowing it to fully charge and then fully discharge during regular use.

ABOUT

Located in Scottsdale, Arizona, Mito Red Light is dedicated to bringing the highest powered, highest quality red light therapy lights to market at the best possible value.

Having extensively studied and realized the benefits of red light therapy firsthand, Mito Red Light was brought into existence in order to provide consumers truly affordable, yet highly effective red light therapy options.

If you have any further questions, please feel free to contact us at:
info@mitoredlight.com

You can also call our phone number

Monday - Friday 9am - 5pm MST
1 (866) 861- MITO

Mail correspondence can be sent to:

Mito Red Light, Inc
9319 N 94th Way,
Suite 400
Scottsdale, AZ 85258

mitoredlight



www.mitoredlight.com

User Manual and Instructional Videos

This user manual and instructional videos can be found here:

<https://mitoredlight.com/pages/user-manual>

Updated March 2024